

# VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100412

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 10/21/2011

## External Standard Test Values

### EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.45: 0.078  
LOT #: 02511080A3  
EXPIRATION: 02/01/2013

BLANK TEST	0.000	22:49
INTERNAL STANDARD	VERIFIED	22:49
EXTERNAL STANDARD	0.077	22:49
BLANK TEST	0.000	22:50
EXTERNAL STANDARD	0.077	22:50
BLANK TEST	0.000	22:51
EXTERNAL STANDARD	0.078	22:51
BLANK TEST	0.000	22:52
EXTERNAL STANDARD	0.078	22:52
BLANK TEST	0.000	22:53
EXTERNAL STANDARD	0.078	22:54
BLANK TEST	0.000	22:54

Average = 0.0776  
Std Dev = 0.0005

## Diagnostic Check

### VERSIONS

DMT: 1.01  
PIC: 3.02  
Modem: 2.0  
Questions: 2.2

### TEMPERATURES

Sample Chamber = 48.7°C	PASSED
Breath Tube = 48.1°C	PASSED

### PUMP INFO

Flow Rate = 5.048 L/M	PASSED
-----------------------	--------

### DETECTOR INFO

PUMP ON	PASSED
PUMP OFF	PASSED


### FILTER INFO

Filter 1	PASSED
Filter 2	PASSED
Filter 3	PASSED

INTERNAL STANDARD	PASSED
-------------------	--------


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

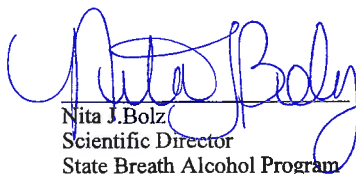 11/4/11  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 4 day of Nov, 20 11

  
Nikki Roth, Notary Public  
My Commission Expires With Office



  
BMMB  
10/27/11